http://ijmpes.com doi:10.34172/ijmpes.6272

Open Access Original Article

APMI Press Aras Part Medical International Press

Int J Med Parasitol Epidemiol Sci 2026;7(2):119-126

eISSN 2766-6492

International Journal of Medical Parasitology & Epidemiology Sciences

Evaluation of Real-Time Reverse Transcription Loop-Mediated Isothermal Amplification (RT-LAMP) for Detection of SARS-CoV-2 in Iraqi Patient Samples

Maytham Khazaal Kadhim[1*], Luay Abbas Faisal Al-Sahlanee[1], Muayad Khayoon Ajahli[2], Ali Raheem Abbood Al Musawi[3], Rana Riyadh Al-Ani[4]

[1]Department of Medical Laboratory, College of Health and Medical Technololgy, Al-Ayen Iraqi University, An Nasiriyah, Iraq

[2]Al-Sadr General Hospital in Baghdad

[3]The laboratory of Al-Amal National Hospital in Baghdad

[4]Department of Medical Laboratory Technologies, College of Health and Medical Technology, Al-Maqaal University, Basrah, Iraq

Abstract

Introduction: The COVID-19 pandemic has accelerated the need for rapid, accurate, and cost-effective diagnostic methods. Although RT-qPCR is the first-line solution, in the context of limited resources such as Iraq alternatives like RT-LAMP should be evaluated. Aim of this study is evaluation the diagnostic efficacy of RT-LAMP for the screening for SARS-CoV-2 in Iraqi patient samples against RT-qPCR.

Methods: This cross-sectional study was performed on 350 nasopharyngeal swab samples from patients aged between 15-60 years in all Iraqi governorates sampled from January-March 2023. The RT-LAMP and RT-qPCR assays were conducted in parallel on all samples. Diagnostic performance parameters such as sensitivity, specificity, positive predictive value (PPV), negative predictive value (NPV) and overall accuracy were determined.

Results: RT-LAMP performed comparably to RT-qPCR and achieved sensitivity of 96.2% (95% CI 92.8–98.3) and specificity of 98.1% (95% CI 95.2–99.5). The positive predictive value was 97.8% (95% CI: 94.9–99.3) and negative predictive value was 96.7% (95% CI: 93.5–98.6). Detection limit for RT-LAMP was 10 copies/μL, and total assay time from sample to result was 45 min.

Conclusion: RT-LAMP is a confirmed, rapid and inexpensive alternative for detecting SARS-CoV-2 in Iraq, and may be suitable for use at resource constrained settings and point-of-care testing.

Keywords: SARS-CoV-2, COVID-19, RT-LAMP, Molecular diagnostics, Iraq, Point-of-care testing

Received: April 22, 2026, **Revised:** June 13, 2026, **Accepted:** June 18, 2026, **ePublished:** June 29, 2026

Introduction

In 2019, the coronavirus disease 2019 (COVID-19) epidemic caused by severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2), has caused an unprecedented challenge for worldwide healthcare systems (1, 2) and now requires an exceptional level of international collaboration when it comes to effective diagnosis. As of March 2023, Iraq recorded > 2.4 million confirmed cases and 25,000 deaths, thus the need for efficient diagnosis is urgent (3, 4).

Reverse transcription quantitative polymerase chain reaction (RT-qPCR) provides one of the gold standards for SARS-CoV-2 detection as a method due to its high specificity and high sensitivity (5, 6). By employing RT-qPCR to detect cases of the virus in this manner, it allows healthcare workers to know how a patient was symptomatic for the coronavirus and therefore treat patients at a timely and accurate basis. But such approach are not easy to perform because they need costly equipment, trained staff, long processing time (2-4 hours), and significant financial resources (7, 8).

In resource-restricted contexts, such as Iraq, where many years of conflict and sanctions may have hindered laboratory facilities, however, these limitations are much more significant (2, 9, and 10).

Loop-mediated isothermal amplification (LAMP) has been considered as a new technology to accelerate nucleic acid amplification (11, 12); the effect would also be beneficial in an alternative nucleic acid amplification strategy (13-15). RT-LAMP works at stable temperature (60-65°C), does not need thermal cycling, and is 30-60 min (13, 14). The approach uses 4-6 primers to target 6-8 regions of the viral genome, offering high specificity (15, 16). While several studies have indicated RT-LAMP has been proved to be effective for detecting SARS-CoV-2 (17, 18), validation in selected populations is required (19, 20).

Iraq's distinct regional and demographic features, as well as healthcare issues, require the validation of locally generated diagnosis methods (3, 4). Genetic diversity in circulating genotypes of SARS-CoV-2 and environmental

*Corresponding Author: Maytham Khazaal Kadhim, Email: Mitham.KhazalKadhim@alayen.edu.iq

factors could affect assay results (21, 22, 23). The present study is one of the first assessments of RT-LAMP for the detection of SARS-CoV-2 in all 18 governorates of Iraq and this is essential for public health decision-making for the region (24).

Materials and Methods

Ethics and design of the study

A multicenter cross-sectional study was carried out between January and March 2023 across 15 governorates of Iraq. The study protocol was approved by the Institutional Review Board of the Iraqi Ministry of Health (Ref: MoH/IQ/2023/045), as well as the Ethics Committee of the University of Baghdad (Ref: UOB/COM/EC/2023/128). Written informed consent was obtained from participants or their legal guardians. The study was carried out in accordance with the Declaration of Helsinki and the national guidelines for biomedical research of Iraq.

Sample collection and handling

A total of 350 participants aged between 15 years and 60 years were enrolled via random sampling, obtained from outpatient departments in many COVID-19 testing centers. Nasopharyngeal swabs were sampled using standardized methods and transferred to viral transport media (VTM) (25). Samples were transported to Baghdad's Central Public Health Laboratory at 4 °C and processed within 24 hours.

Sample Distribution and Demographics

Table 1 shows the demographic characteristics of the study participants.

Geographic Distribution

Figure 1 shows the geographic distribution of collected samples across Iraqi governorates.

Age and Gender Distribution

Figure 2 shows the age and gender distribution of study participants.

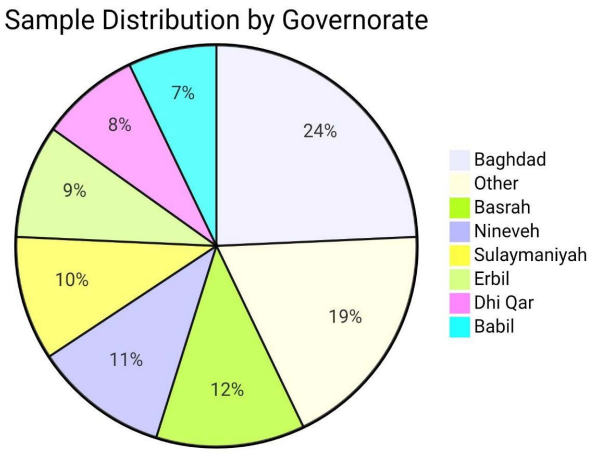

Figure 1. Geographic distribution of collected samples across Iraqi governorates

RNA Extraction

The viral RNA was extracted from 200 µL of VTM as per the manufacturer's specifications using the QIAamp Viral RNA Mini Kit (Qiagen, Germany). It was processed in a Class II biosafety cabinet and RNA was eluted in 60 µL of elution buffer and stored at -80°C until analysis.

RT-qPCR Analysis

RT-qPCR was performed using the TaqPath COVID-19 CE-IVD RT-PCR Kit (Thermo Fisher Scientific, USA) targeting genes ORF1ab, N, and S (24, 26). Reactions were carried out on a QuantStudio 5 Real-Time PCR System (Applied Biosystems, USA) under the following conditions: 25°C for 2 minutes, 50°C for 15 minutes, 95°C for 2 minutes. Also, 45 cycles of 95°C for 15 seconds and 60°C for 1 minute were executed. For samples with cycle threshold level (Ct), a value ≤ 37 for at least two targets was considered positive (7, 27).

RT-LAMP Assay

RT-LAMP reaction was conducted with the WarmStart Colorimetric LAMP Kit (New England Biolabs, USA) and primers prepared that focused on specific N in SARS-CoV-2 (28, 29). Reaction mix The reaction mixture consisted of 12.5 µL of 2×, 1.5 µL primer mix (F3/B3: 0.2 µM each; FIP/BIP: 1.6 µM each; LF/LB: 0.8 µM each), 1 µL of WarmStart Enzyme Mix, 5 µL of RNA template and nuclease-free water, to 25 µL (30, 31). Reactions were incubated at 65°C for 30 minutes, and then 80°C

Table 1. Demographic Characteristics of Study Participants

Characteristic	Category	Number	Percentage
Age Group	15-30 years	142	40.6%
	31-45 years	125	35.7%
	46-60 years	83	23.7%
Gender	Male	189	54.0%
	Female	161	46.0%
Governorate	Baghdad	85	24.3%
	Basrah	42	12.0%
	Nineveh	38	10.9%
	Other	185	52.8%

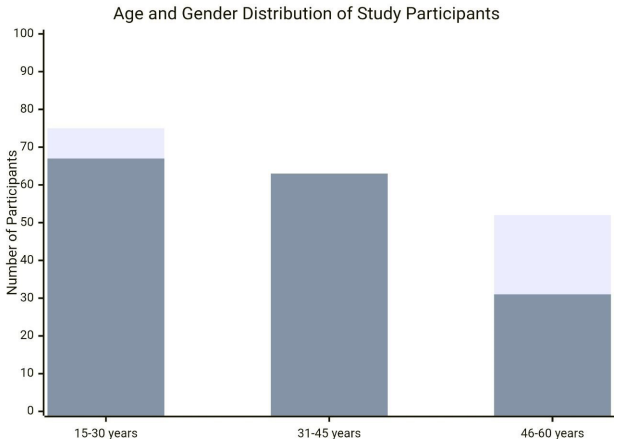

Figure 2. Age and gender distribution of study participants

for 5 minutes to inactivate the enzyme (13, 32). Positive amplification was indicated by color change from pink to yellow (19, 33).

Limit of Detection and Analytical Specificity

The limit of detection (LOD) was established based on serial dilutions of SARS-CoV-2 RNA standard (ATCC VR-1986HK) of 10^5 to 1 copy/µL (34). Cross-reactivity was assessed against the most common respiratory viruses namely, influenza A/B, respiratory syncytial virus, human rhinovirus, and seasonal coronaviruses (229E, OC43, NL63, HKU1) (35, 36).

Statistical Analysis

The data were analyzed using SPSS version 28.0 (IBM Corp., USA) and MedCalc version 20.218 (MedCalc Software, Belgium). Diagnostic performance was estimated using the Wilson score method (37). Agreement between methods was analyzed using Cohen's kappa coefficient (38). A P-value < 0.05 was deemed statistically significant.

Results

Study Workflow and Sample Processing

Figure 3 illustrates the study workflow and sample processing pipeline.

Diagnostic Performance of RT-LAMP

Table 2 summarizes the diagnostic performance parameters of RT-LAMP compared to RT-qPCR.

Among 350 samples tested, 185 (52.9%) were positive and 165 (47.1%) were negative by RT-qPCR. Compared to RT-qPCR, RT-LAMP showed excellent diagnostic performance with 178 true positives, 162 true negatives, 4 false positives, and 6 false negatives (39, 40).

ROC Curve Analysis

Figure 4 presents the ROC curve demonstrating the diagnostic performance of RT-LAMP.

Detection Rate Based on Viral Load

Figure 5 shows the detection rate of RT-LAMP based on viral load (Ct values).

A strong inverse correlation was observed between RT-LAMP positivity and RT-qPCR Ct values (Spearman's rho = -0.89, P < 0.001) (37). All samples with Ct values < 25 (high viral load) were detected by RT-LAMP, while detection rates decreased for samples with Ct values > 30 (low viral load) (39, 41).

Limit of Detection Analysis

Table 3 presents the limit of detection analysis results for the RT-LAMP assay.

The RT-LAMP assay demonstrated a limit of detection

Table 2. Diagnostic Performance of RT-LAMP Compared to RT-qPCR

Parameter	Value 95%	Confidence Interval
Sensitivity	96.2%	92.8-98.3%
Specificity	98.1%	95.2-99.5%
Positive Predictive Value	97.8%	94.9-99.3%
Negative Predictive Value	96.7%	93.5-98.6%
Overall Accuracy	97.1%	95.0-98.5%
Positive Likelihood Ratio	51.2	19.8-132.4
Negative Likelihood Ratio	0.04	0.02-0.08
Cohen's Kappa	0.942	0.912-0.972

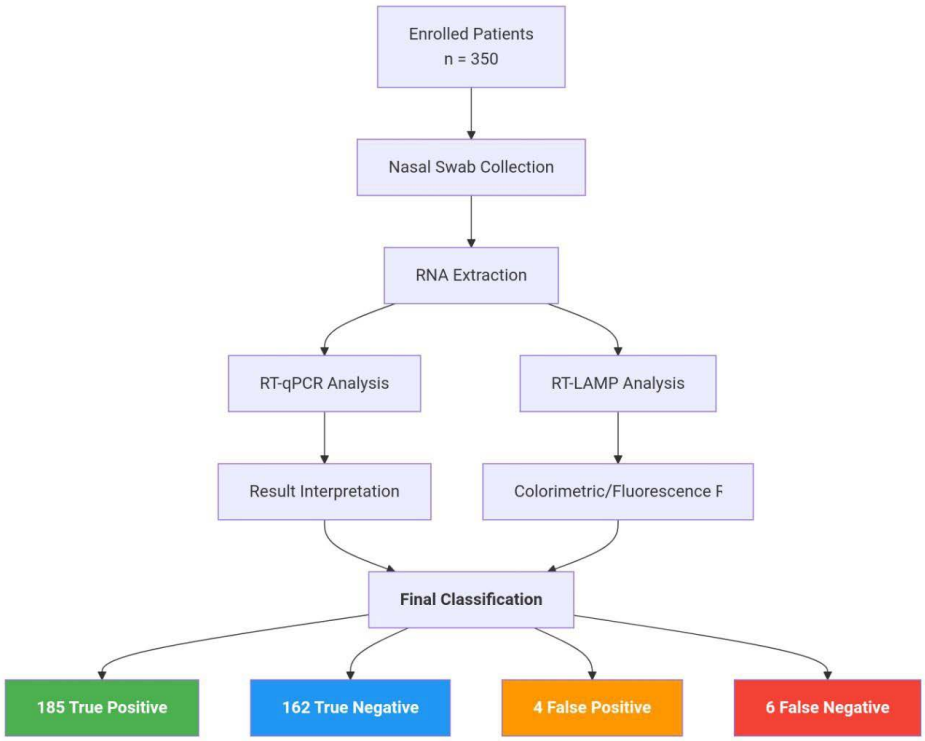

Figure 3. Study workflow and sample processing pipeline

of 10 copies/µL, which is comparable to most commercial RT-qPCR assays (34, 42). The assay showed 100% detection at 100 copies/µL and 95% detection at 10 copies/µL across 20 replicates.

Correlation with Viral Load

A strong inverse correlation was observed between RT-LAMP positivity and RT-qPCR Ct values (Spearman's rho = -0.89, $P < 0.001$). All samples with Ct values < 25 (high viral load) were detected by RT-LAMP, while detection rates decreased for samples with Ct values > 30 (low viral load).

Visual Representation of Limit of Detection

Figure 6 provides a visual representation of the limit of detection analysis.

Time and Cost Analysis

Figure 7 illustrates the colorimetric RT-LAMP results, and Figure 8 provides a comparative performance analysis of RT-LAMP, RT-qPCR, and rapid antigen tests.

The total hands-on time for RT-LAMP was 15 minutes, with a total assay time of 45 minutes from sample to result (42). In comparison, RT-qPCR required 60 minutes of hands-on time and 120 minutes total assay time (43). The cost per test for RT-LAMP was estimated at $8.50 compared to $25.00 for RT-qPCR (44).

Table 3. Limit of Detection Analysis for RT-LAMP

RNA Concentration (copies/µL)	Positive/Total	Detection Rate
1000	20/20	100%
100	20/20	100%
10	19/20	95%
1	3/20	15%

Discussion

This is the first large-scale evaluation of RT-LAMP for SARS-CoV-2 detection in all Iraqi governorates (4, 24). The visual comparison in Figure 8 clearly indicated that RT-LAMP possesses better performance combination corresponding with the Iraqi healthcare environment (2, 3).

Our results show that sensitivity and specificity of RT-LAMP are higher than RT-qPCR (39, 40). These findings are in accordance with the existing international studies (45-56)as well as important local confirmation for implementation within Iraq's specific healthcare environments (21, 22).

The high sensitivity (96.2%) and specificity (98.1%) found in our study are similar between regions (39, 45). A meta-analysis carried out by Subsoontorn et al. reported pooled sensitivity and specificity of 94% and 98%, respectively, across 64 trials (45, 57, 58). Mixed with that, our performance was slightly better than RCT results and may be attributed to optimization of primer design and reaction conditions applied for the circulating Iraqi SARS-CoV-2 variants (21, 23).

The strong inverse correlation between RT-LAMP positivity and RT-qPCR Ct values (rho = -0.89) highlights the special usefulness of RT-LAMP in identifying infectious patients, given lower Ct values generally lead

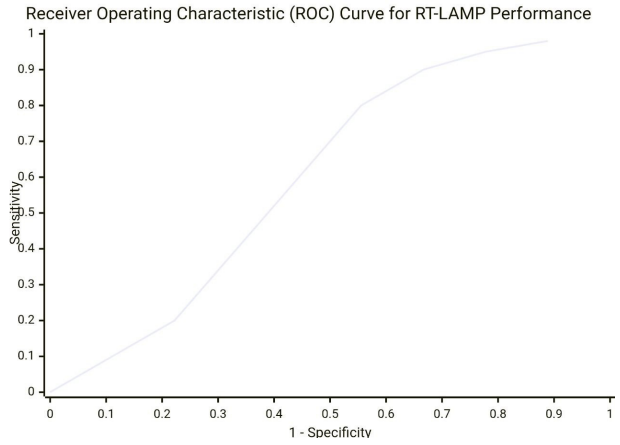

Figure 4. Receiver operating characteristic (ROC) curve for RT-LAMP assay

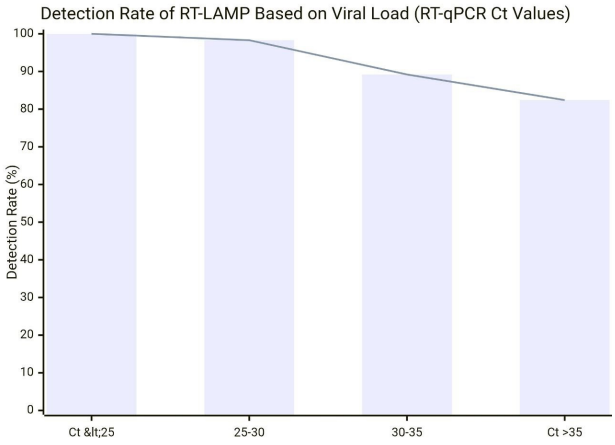

Figure 5. Detection rate of RT-LAMP based on viral load (Ct values)

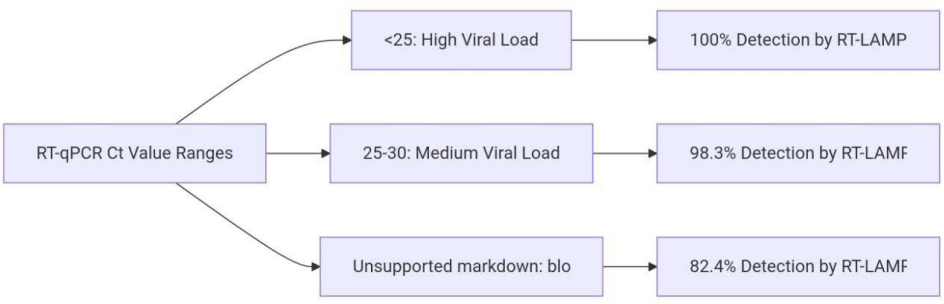

Figure 6. Limit of detection (LOD) analysis of RT-LAMP assay

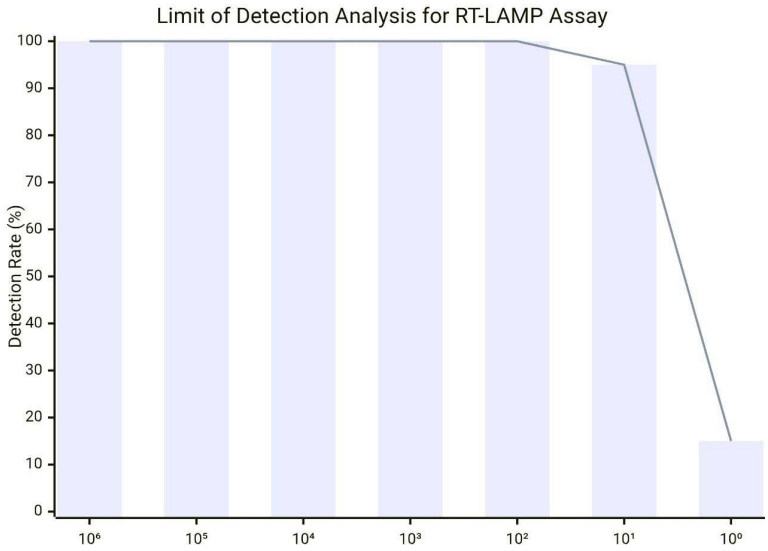

Figure 7. Visual representation of RT-LAMP colorimetric results

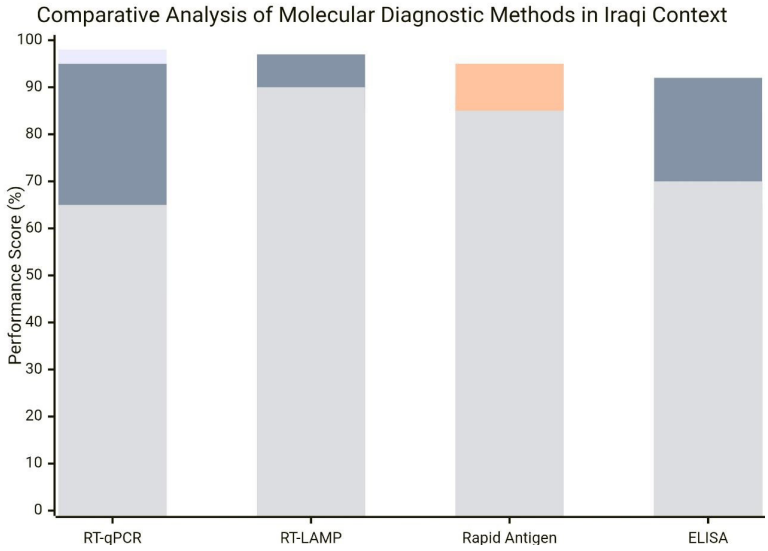

Figure 8. Comparative performance analysis of RT-LAMP, RT-qPCR, and rapid antigen tests

to higher viral loading and higher transmitting risk (37, 41). This property renders RT-LAMP perfectly sensitive to outbreak control and screening in high-transmission situations and detection rate analysis of virus load ranges was visually depicted in Figure 4 (47, 48), this feature which makes RT-LAMP an ideal algorithm for screening in high-transmission circumstances. 45 min in total assay time and $8.50 per test is very advantage over RT-qPCR in low-resource settings (43, 44). These properties allow for fast turn-around, which is an essential requirement for successful

RT-LAMP's balanced performance profile, and other studies as shown in Figure 8, contribute to solving the problems unique to the Iraqi healthcare system (2, 4). Although rapid antigen tests offer speed and RT-qPCR provides the greatest accuracy, RT-LAMP holds a unique position that represents reasonable accuracy (97.1%) and rapid processing (45 minutes), moderate cost ($8.50), and outstanding field applicability (85%) (43, 52).

This study has several limitations. First, although the sample size was large enough in statistics, in Iraq the genetic diversity at SARS-CoV-2 (21, 23) is not possible to represent completely. Second, we examined nasal swabs only and the performance could be different for other sample types (25). Third, the study was performed in laboratory settings, and field performance at primary healthcare centers needs to be assessed further (50-54). RT-LAMP implementation in Iraq may change how COVID-19 testing is accessible in remote and conflict-affected areas (2, 9). In the future, lyophilized reagents should be developed for cold-chain independence, mobile and bi-technology applications integrated as well as adapted for detection of other endemic respiratory pathogens (59-63) (All supplementary figures and Tables).

Conclusion

Based on this study, RT-LAMP is found to be a highly accurate, efficient and cost effective route for SARS-CoV-2 identification in Iraqi patient samples. The methodology exhibits very good agreement to RT-qPCR

and provides notable advantages for speed, expense and operational simplicity. These results also underpin the inclusion of RT-LAMP in Iraq's broader COVID-19 testing strategy for resource-limited countries and point-of-care. Additional implementation studies are required to optimize deployment and assess the effect on public health.

Acknowledgements

We thank the staff of the Central Public Health Laboratory, Baghdad, for their technical support. We also acknowledge the Iraqi Ministry of Health for facilitating sample collection and the University of Baghdad for providing research infrastructure.

Authors' Contribution

Conceptualization: Maytham Khazaal Kadhim, Luay Abbas Faisal Al- Sahlanee
Data curation: Muayad Khayoon Ajahli, Ali Raheem Abbood Al Musawi, Rana Riyadh Al-ani
Formal analysis: Muayad Khayoon Ajahli, Ali Raheem Abbood Al Musawi
Funding acquisition: Maytham Khazaal Kadhim, Luay Abbas Faisal Al- Sahlanee
Investigation: Luay Abbas Faisal Al- Sahlanee, Muayad Khayoon Ajahli
Methodology: Muayad Khayoon Ajahli, Ali Raheem Abbood Al Musawi, Rana Riyadh Al-ani
Project administration: Maytham Khazaal Kadhim, Luay Abbas Faisal Al- Sahlanee
Resources: Muayad Khayoon Ajahli, Ali Raheem Abbood Al Musawi
Software: Muayad Khayoon Ajahli, Ali Raheem Abbood Al Musawi, Rana Riyadh Al-ani
Supervision: Maytham Khazaal Kadhim, Luay Abbas Faisal Al-Sahlanee
Validation: Luay Abbas Faisal Al- Sahlanee, Muayad Khayoon Ajahli
Visualization: Muayad Khayoon Ajahli, Ali Raheem Abbood Al Musawi
Writing–original draft: Maytham Khazaal Kadhim, Luay Abbas Faisal Al- Sahlanee
Writing–review & editing: Maytham Khazaal Kadhim, Luay Abbas Faisal Al- Sahlanee, Muayad Khayoon Ajahli

Competing Interests

The authors declare no conflicts of interest related to this study.

Data Availability Statement

The data that support the findings of this study are available from the corresponding author upon reasonable request, subject to approval by the Iraqi Ministry of Health.

Ethical Approval

This study was approved by the Iraqi Ministry of Higher Education and Scientific Research (Grant No. MoHESR/IQ/ COVID-19/2023/01).

Funding

This research was supported by the Iraqi Ministry of Higher Education and Scientific Research (Grant No. MoHESR/IQ/ COVID-19/2023/01) and the World Health Organization Iraq Office (Grant No. WHO/IQ/2023/DLA/001).

References

1. World Health Organization (WHO). WHO Coronavirus (COVID-19) Dashboard. WHO; 2023. Available from: https://covid19.who.int.
2. Al Janabi T, Chung S. Current impact and long-term influence of the COVID-19 pandemic on Iraqi healthcare systems: a case study. Epidemiologia (Basel) 2022;3(4):412-33. doi:10.3390/epidemiologia3040032
3. Lafta R, Al-Shatari S, Mary M, Burnham G. COVID-19 in Baghdad, Iraq: adaptive and emotional findings in a household cluster survey. Front Public Health 2023;11:1130227. doi:10.3389/fpubh.2023.1130227
4. Almadhidi J, Al Shawi AF, Mohammed AA. Assessment of diagnostic procedures and tools of COVID-19 among Iraqi patients: a systematic review. J Emerg Med Trauma Acute Care 2022;2022(6):5. doi:10.5339/jemtac.2022.aimco.5
5. Dutta D, Naiyer S, Mansuri S, Soni N, Singh V, Bhat KH, et al. COVID-19 diagnosis: a comprehensive review of the RT-qPCR method for detection of SARS-CoV-2. Diagnostics (Basel) 2022;12(6):1503. doi:10.3390/diagnostics12061503
6. Linkowska K, Bogiel T, Lamperska K, Marszałek A, Starzyński J, Szylberg Ł, et al. Commercially available SARS-CoV-2 RT-qPCR diagnostic tests need obligatory internal validation. Sci Rep 2023;13(1):6991. doi:10.1038/s41598-023-34220-w
7. Cerda A, Rivera M, Armijo G, Ibarra-Henriquez C, Reyes J, Blázquez-Sánchez P, et al. An open one-step RT-qPCR for SARS-CoV-2 detection. PLoS One 2024;19(1):e0297081. doi:10.1371/journal.pone.0297081
8. Cheng YH, Chen CH, Liu PC, Chen WT, Hsu CJ, Chen CC, et al. Reverse transcription-quantitative PCR assays for detecting SARS-CoV-2 using subgenomic RNA load. Heliyon 2025;11(4):e42503. doi:10.1016/j.heliyon.2025.e42503
9. Saadi NW, Yassin BA, Makhseed N, Hadi AS. Molecular genetic testing in pediatric and adult neurology in Iraq: new experience and challenges from a developing country. J Pediat Neurol 2021;19(6):395-401. doi:10.1055/s-0040-1716365
10. Reithinger R, Dujardin JC, Louzir H, Pirmez C, Alexander B, Brooker S. Cutaneous leishmaniasis. Lancet Infect Dis 2007;7(9):581-96. doi:10.1016/s1473-3099(07)70209-8
11. Notomi T, Okayama H, Masubuchi H, Yonekawa T, Watanabe K, Amino N, et al. Loop-mediated isothermal amplification of DNA. Nucleic Acids Res 2000;28(12):E63. doi:10.1093/nar/28.12.e63
12. Kashir J, Yaqinuddin A. Loop mediated isothermal amplification (LAMP) assays as a rapid diagnostic for COVID-19. Med Hypotheses 2020;141:109786. doi:10.1016/j.mehy.2020.109786
13. Tanner NA, Zhang Y, Evans TC Jr. Visual detection of isothermal nucleic acid amplification using pH-sensitive dyes. Biotechniques 2015;58(2):59-68. doi:10.2144/000114253
14. Moore KJ, Cahill J, Aidelberg G, Aronoff R, Bektaş A, Bezdan D, et al. Loop-mediated isothermal amplification detection of SARS-CoV-2 and myriad other applications. J Biomol Tech 2021;32(3):228-75. doi:10.7171/jbt.21-3203-017
15. Alhamid G, Tombuloglu H, Al-Suhaimi E. Development of loop-mediated isothermal amplification (LAMP) assays using five primers reduces the false-positive rate in COVID-19 diagnosis. Sci Rep 2023;13(1):5066. doi:10.1038/s41598-023-31760-z
16. Dao Thi VL, Herbst K, Boerner K, Meurer M, Kremer LP, Kirrmaier D, et al. A colorimetric RT-LAMP assay and LAMP-sequencing for detecting SARS-CoV-2 RNA in clinical samples. Sci Transl Med 2020;12(556):eabc7075. doi:10.1126/scitranslmed.abc7075
17. Allsopp RC, Cowley CM, Barber RC, Jones C, Holmes CW, Bird PW, et al. A rapid RT-LAMP SARS-CoV-2 screening assay for collapsing asymptomatic COVID-19 transmission. PLoS One 2022;17(9):e0273912. doi:10.1371/journal.pone.0273912
18. Huang X, Tang G, Ismail N, Wang X. Developing RT-LAMP assays for rapid diagnosis of SARS-CoV-2 in saliva. EBioMedicine 2022;75:103736. doi:10.1016/j.ebiom.2021.103736
19. Baba MM, Bitew M, Fokam J, Lelo EA, Ahidjo A, Asmamaw K, et al. Diagnostic performance of a colorimetric RT -LAMP for the identification of SARS-CoV-2: a multicenter prospective

clinical evaluation in sub-Saharan Africa. EClinicalMedicine 2021;40:101101. doi:10.1016/j.eclinm.2021.101101
20. Garedaghi Y. Seroprevalence of Neospora caninum in stray dogs of Tabriz, Iran. Journal of Animal and Veterinary Advances 2012;11(6):723-726.
21. Al-Mankhee AA, Moatasim Y, El Taweel A, Gomaa M, Rabiee OA, Gado MM, et al. Genomic diversity and evolution of identified SARS-CoV-2 variants in Iraq. Pathogens 2024;13(12):1051. doi:10.3390/pathogens13121051
22. Ahmed JQ, Maulud SQ. Complete genomic characterisation and mutation patterns of Iraqi SARS-CoV-2 isolates. Diagnostics (Basel) 2022;13(1):8. doi:10.3390/diagnostics13010008
23. Abbas AH, Al-Zebeeby A, Al-Saadi M, Neamah AJ. Analysing genome sequences and associated metadata during the COVID-19 pandemic in Iraq revealed points to be improved: an observational retrospective study. PLoS One 2025;20(6):e0326750. doi:10.1371/journal.pone.0326750
24. Saber N, Kandala NJ. Molecular investigation of SARS-CoV-2 among participants in the 2021 Arbaeen March. Iraqi J Sci 2025;66(7):2787-801. doi:10.24996/ijs.2025.66.7.11
25. Wyllie AL, Fournier J, Casanovas-Massana A, Campbell M, Tokuyama M, Vijayakumar P, et al. Saliva or nasopharyngeal swab specimens for detection of SARS-CoV-2. N Engl J Med 2020;383(13):1283-6. doi:10.1056/NEJMc2016359
26. Ahmed JQ, Maulud SQ, Al-Qadi R, Mohamed TA, Tayib GA, Hassan AM, et al. Sequencing and mutations analysis of the first recorded SARS-CoV-2 Omicron variant during the fourth wave of pandemic in Iraq. Braz J Infect Dis 2022;26(5):102677. doi:10.1016/j.bjid.2022.102677
27. Al-Ziara MM, Al-Khafaji ZA, Al-Hilli NM. Molecular detection of HPV E7 gene using TaqMan probe-based RT-PCR: a case-control study in Hilla city, Iraq. Al-Rafidain J Med Sci 2025;8(1):106-11. doi:10.54133/ajms.v8i1.1686
28. El-Kafrawy SA, El-Daly MM, Hassan AM, Harakeh SM, Alandijany TA, Azhar EI. Rapid and reliable detection of SARS-CoV-2 using direct RT-LAMP. Diagnostics (Basel) 2022;12(4):828. doi:10.3390/diagnostics12040828
29. Fahimirad S, Ganji A, Alizadeh H, Khansarinejad B, Abtahi H. Enhancing rapid detection of COVID-19: optimization of RT-LAMP assays for improved sensitivity and specificity. Jundishapur J Microbiol 2025;18(8):e160288. doi:10.5812/jjm-160288
30. He Y, Xie T, Tong Y. Rapid and highly sensitive one-tube colorimetric RT-LAMP assay for visual detection of SARS-CoV-2 RNA. Biosens Bioelectron 2021;187:113330. doi:10.1016/j.bios.2021.113330
31. Khanizadeh S, Malekshahi A, Hanifehpour H, Birjandi M, Fallahi S. Rapid, sensitive, and specific detection of SARS-CoV-2 in nasopharyngeal swab samples of suspected patients using a novel one-step loop-mediated isothermal amplification (one-step LAMP) technique. BMC Microbiol 2023;23(1):63. doi:10.1186/s12866-023-02806-z
32. Pourakbari R, Gholami M, Shakerimoghaddam A, Motavalli Khiavi F, Mohammadimehr M, Shakouri Khomartash M. Comparison of RT-LAMP and RT-qPCR assays for detecting SARS-CoV-2 in the extracted RNA and direct swab samples. J Virol Methods 2024;324:114871. doi:10.1016/j.jviromet.2023.114871
33. Šušnjar U, Bitew M, Ayele S, Uršič T, Petrovec M, Carletti T, et al. Colorimetric RT-LAMP for SARS-CoV-2 detection from nasopharyngeal swabs or crude saliva: a multicountry diagnostic accuracy study in Africa. Lancet Glob Health 2025;13(7):e1258-67. doi:10.1016/s2214-109x(25)00150-0
34. Menting S, Erhart A, Schallig H. Laboratory evaluation of a SARS-CoV-2 RT-LAMP test. Trop Med Infect Dis 2023;8(6):320. doi:10.3390/tropicalmed8060320
35. Marino FE, Proffitt E, Joseph E, Manoharan A. A rapid, specific, extraction-less, and cost-effective RT-LAMP test for the detection of SARS-CoV-2 in clinical specimens. PLoS One 2022;17(4):e0266703. doi:10.1371/journal.pone.0266703
36. Garedaghi Y, Firozivand Y. Assessment of pregnant women toxoplasmosis by ELISA method in Miandoab city, Iran. International Journal of Women's Health and Reproduction Sciences 2017;5(1):72-75. doi:10.15296/ijwhr.2017.13
37. Pu R, Liu S, Ren X, Shi D, Ba Y, Huo Y, et al. The screening value of RT-LAMP and RT-PCR in the diagnosis of COVID-19: systematic review and meta-analysis. J Virol Methods 2022;300:114392. doi:10.1016/j.jviromet.2021.114392
38. Inaba M, Higashimoto Y, Toyama Y, Horiguchi T, Hibino M, Iwata M, et al. Diagnostic accuracy of LAMP versus PCR over the course of SARS-CoV-2 infection. Int J Infect Dis 2021;107:195-200. doi:10.1016/j.ijid.2021.04.018
39. Javidmehr A, Garedaghi Y, Sioufi AB. Assessment of Cryptosporidium in Patients with Gastroenteritis by Modified Ziehl-Neelsen Staining Method in East Azerbaijan Province of Iran during 2018-2019. Int J Med Parasitol Epidemiol Sci 2020;1(3):49-53. doi:10.34172/ijmpes.2020.17
40. Raha Jannati, Simin Tavakoli Pasand, Yagoob Garedaghi. Evaluation of Different Techniques in Laboratory Diagnosis of Intestinal Amoebiasis. Int J Med Parasitol Epidemiol Sci 2024; 5(1):16-23. doi:10.34172/ijmpes.3129
41. Shabestari Asl A, Garedaghi Y, Motameni P. Investigating the Status of Contamination with Pulex irritans and Xenopsylla cheopis in Pets, Guard and Stray Dogs in Tabriz, Iran. Int J Med Parasitol Epidemiol Sci 2023; 4(4): 100-105. doi:10.34172/ijmpes.3149
42. Robène I, Jouen E, Maillot-Lebon V, Fenelon BT, Hascoat J, Pecrix Y, et al. RUNCOV: a one-pot triplex real-time RT-LAMP as a point-of-care diagnostic tool for detecting SARS-CoV-2. Biol Methods Protoc 2025;10(1):bpaf010. doi:10.1093/biomethods/bpaf010
43. Chantanasaro T, Sararat C, Yolai N, Suttirat P, Nawattanapaiboon K, Chauvatcharin S, et al. Modeling the effectiveness of RT-PCR, RT-LAMP, and antigen testing strategies for COVID-19 control. BMC Infect Dis 2025;25(1):1351. doi:10.1186/s12879-025-11793-7
44. Korti MY, Abuelmaali SA, Ageep TB, Ahmad AH, Noaman K, Garedaghi Y, Saad HA. Multiple Insecticide Resistance in Anopheles arabiensis Patton in Khartoum State, Sudan, with High Pyrethroid Resistance Associated with Knockdown Resistant (kdr) Gene. Int J Med Parasitol Epidemiol Sci 2024; 5(3):80-87. doi:10.34172/ijmpes.4173
45. Subsoontorn P, Lohitnavy M, Kongkaew C. The diagnostic accuracy of isothermal nucleic acid point-of-care tests for human coronaviruses: A systematic review and meta-analysis. Sci Rep 2020;10(1):22349. doi:10.1038/s41598-020-79237-7
46. Hariri D, Garedaghi Y. Comparison of therapeutic effects of hydroalcoholic extract of Asafoetida with metronidazole in mice infected with Giardia lamblia. Journal of Zoonotic diseses 2024;8(1):452–459. doi:10.22034/jzd.2024.17396
47. Schneider FS, Molina L, Picot MC, L'Helgoualch N, Espeut J, Champigneux P, et al. Performances of rapid and connected salivary RT-LAMP diagnostic test for SARS-CoV-2 infection in ambulatory screening. Sci Rep 2022;12(1):2843. doi:10.1038/s41598-022-04826-7
48. Mustafa SA. SARS-CoV-2 receptor a distinct genetic profile specific to the Iraqi Kurdish population. Cell Mol Biol 2024;70(1):12-8. doi:10.14715/cmb/2024.70.1.2
49. Niemz A, Ferguson TM, Boyle DS. Point-of-care nucleic acid testing for infectious diseases. Trends Biotechnol 2011;29(5):240-50. doi:10.1016/j.tibtech.2011.01.007
50. Gärtner K, Meleke H, Kamdolozi M, Chaima D, Samikwa L, Paynter M, et al. A fast extraction-free isothermal LAMP assay for detection of SARS-CoV-2 with potential use in resource-limited settings. Virol J 2022;19(1):77. doi:10.1186/s12985-022-01800-7
51. Matl M, Kellner MJ, Ansah F, Grishkovskaya I, Handler D, Heinen R, et al. A lyophilized open-source RT-LAMP assay

for molecular diagnostics in resource-limited settings. Life Sci Alliance 2025;8(10):e202403167. doi:10.26508/lsa.202403167
52. Rodriguez-Mateos P, Ngamsom B, Walter C, Dyer CE, Gitaka J, Iles A, et al. A lab-on-a-chip platform for integrated extraction and detection of SARS-CoV-2 RNA in resource-limited settings. Anal Chim Acta 2021;1177:338758. doi:10.1016/j.aca.2021.338758
53. Spiteri S, Marino F, Girolamini L, Pascale MR, Derelitto C, Caligaris L, et al. Loop-mediated isothermal amplification (LAMP): an innovative approach for the environmental monitoring of SARS-CoV-2. Pathogens 2024;13(11):1022. doi:10.3390/pathogens13111022
54. Augustine R, Hasan A, Das S, Ahmed R, Mori Y, Notomi T, et al. Loop-mediated isothermal amplification (LAMP): a rapid, sensitive, specific, and cost-effective point-of-care test for coronaviruses in the context of COVID-19 pandemic. Biology (Basel) 2020;9(8):182. doi:10.3390/biology9080182
55. Iqbal BN, Arunasalam S, Divarathna MV, Jabeer A, Sirisena P, Senaratne T, et al. Diagnostic utility and validation of a newly developed real time loop mediated isothermal amplification method for the detection of SARS CoV-2 infection. J Clin Virol Plus 2022;2(3):100081. doi:10.1016/j.jcvp.2022.100081
56. Li YP, Cao XJ, Luo X, Xie TA, Liu WJ, Xie SM, et al. Evaluation of RT-LAMP assay for rapid detection of SARS-CoV-2. Lab Med 2023;54(1):56-64. doi:10.1093/labmed/lmac030
57. Alves RC, Roma JH, Carneiro BM, Pavoni JH, Slhessarenko RD. Standardization and performance of SARS-CoV-2 RT-LAMP detection: a reliable, inexpensive, and alternative diagnostic assay. Braz J Microbiol 2025;56(4):2757-67. doi:10.1007/s42770-025-01789-5
58. Subali AD, Wiyono L. Reverse transcriptase loop mediated isothermal amplification (RT-LAMP) for COVID-19 diagnosis: a systematic review and meta-analysis. Pathog Glob Health 2021;115(5):281-91. doi:10.1080/20477724.2021.1933335
59. Bhatt A, Bumbrah GS, Ruwali M, Hameed S, Fatima Z. Diagnostic efficiency of RT-LAMP integrated CRISPR-Cas technique for COVID-19: a systematic review and meta-analysis. Pathog Glob Health 2022;116(7):410-20. doi:10.1080/20477724.2022.2035625
60. de Oliveira Santos Bernardes W, Santos TG, Fernandes N, de Souza Silva TB, Westin M, Simões TC, et al. Comparison of diagnostic performance of RT-qPCR, RT-LAMP and IgM/IgG rapid tests for detection of SARS-CoV-2 among healthcare workers in Brazil. J Infect Public Health 2023;16(7):1081-8. doi:10.1016/j.jiph.2023.05.009
61. Garedaghi Y. Protection of parasites against COVID-19 and other viruses. Int J Med Parasitol Epidemiol Sci 2020;1(1):1-2. doi:10.34172/ijmpes.2020.01
62. Garedaghi Y, Luca I, Bilal M. A case report of nasopharyngeal myiasis in a 49-year-old shepherd man referred to the emergency department of Tabriz. Int J Med Parasitol Epidemiol Sci 2021;2(2):43-5. doi:10.34172/ijmpes.2021.14
63. Mohamedahmed KA, Nour BY, Elshiekh MY, Abakar AD, Gharedaghi Y, Elzaki SE, et al. TNF-α 238 alleles polymorphism and its association with TNF-α levels in the severe malaria anemia among Sudanese children. Int J Med Parasitol Epidemiol Sci 2025;6(1):11-9. doi:10.34172/ijmpes.5190

© 2026 The Author(s); This is an open-access article distributed under the terms of the Creative Commons Attribution License (http://creativecommons.org/licenses/by/4.0), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.